

An experimental evaluation of fracture movement in two alternative tibial fracture fixation models using a vibrating platform

Mehran Moazen¹ , Peter Calder², Paul Koroma², Jonathan Wright² , Stephen Taylor² and Gordon Blunn^{2,3}

Proc IMechE Part H:
J Engineering in Medicine
2019, Vol. 233(5) 595–599
© IMechE 2019
Article reuse guidelines:
sagepub.com/journals-permissions
DOI: 10.1177/0954411919837304
journals.sagepub.com/home/pih


Abstract

Several studies have investigated the effect of low-magnitude-high-frequency vibration on the outcome of fracture healing in animal models. The aim of this study was to quantify and compare the micromovement at the fracture gap in a tibial fracture fixed with an external fixator in both a surrogate model of a tibial fracture and a cadaver human leg under static loading, both subjected to vibration. The constructs were loaded under static axial loads of 50, 100, 150 and 200 N and then subjected to vibration at each load using a commercial vibration platform, using a DVRT sensor to quantify static and dynamic fracture movement. The overall stiffness of the cadaver leg was significantly higher than the surrogate model under static loading. This resulted in a significantly higher fracture movement in the surrogate model. Under vibration, the fracture movements induced at the fracture gap in the surrogate model and the cadaver leg were 0.024 ± 0.009 mm and 0.016 ± 0.002 mm, respectively, at 200 N loading. Soft tissues can alter the overall stiffness and fracture movement recorded in biomechanical studies investigating the effect of various devices or therapies. While the relative comparison between the devices or therapies may remain valid, absolute magnitude of recordings measured externally must be interpreted with caution.

Keywords

Biomechanics, fracture fixation, stiffness, fracture movement, external fixator, cadaver, tibiae, non-union

Date received: 27 August 2017; accepted: 11 February 2019

Introduction

Ilizarov Frame hexapods of various design are typically used in the management of long bone fractures in the field of orthopaedic trauma. Non-union fractures remain a challenge however, and account for around 10% of all fractures treated and about 2% of tibial diaphyseal fractures.^{1–3} There are several contributing factors to non-union including the patient, injury and treatment protocols.^{2,3} The stability of initial fracture fixation and post-operative loading of the fracture are among the key treatment-related factors.^{4–13} Both contribute to the mechanobiology of the healing fracture where it is well established that there are certain strain thresholds that promote callus formation. For example, interfragmentary motion (IFM) in the range of 0.2–1 mm and 2%–10% strain is suggested to improve fracture healing.^{4,5,11,12}

There are some studies suggesting that the application of low-intensity pulsed ultrasound (LIPUS) and

whole body vibration (WBV) may possibly improve fracture healing and potentially address non-union.^{14–19} The exact mechanisms by which these methods improve fracture healing at the molecular and cellular level are still unknown. However, it is generally accepted that LIPUS generates nano-scale motions while WBV generates micro-scale motion at the fracture site leading to different mechanisms of improved healing.

¹Department of Mechanical Engineering, University College London, London, UK

²Institute of Orthopaedics and Musculoskeletal Science, Division of Surgery & Interventional Science, University College London, Royal National Orthopaedic Hospital, Stanmore, UK

³School of Pharmacy and Biomedical Sciences, University of Portsmouth, Portsmouth, UK

Corresponding author:

Mehran Moazen, Department of Mechanical Engineering, University College London, Torrington Place, London WC1E 7JE, UK.
Email: M.Moazen@ucl.ac.uk

There has been no prior study to quantify the movement induced at the fracture gap as a result of external vibration in a tibial fracture fixed with an external fixator. Surrogate bone models and cadaveric tissue can be used to compare the fracture movement in an *in vitro* study. An *in vitro* fixation of a surrogate bone in the absence of soft tissues should provide little attenuation to vibration applied at the foot when observed at the fracture gap. While, in a cadaver model, the magnitude of the displacement induced by the vibrating platform at the foot may be attenuated by the presence of the soft tissues. Incremental fracture displacements of 1 mm/day are usually induced clinically using an external frame, although the soft tissues and bone remodelling stiffness determine the actual mode of distraction at the fracture gap. In this study, we were not able to replicate the bone remodelling response, but just the soft tissues. However, the growing bone formed during distraction osteogenesis would have a low modulus of elasticity compared to mature bone.

The aim of this study was to quantify and compare the micromovement at the fracture gap in a tibial fracture fixed with an external fixator in both a surrogate model and cadaver leg under both static loading and subject to vibration. Therefore, the study quantifies and compares the overall stiffness and fracture movement in both models, and investigates if comparable trends exist between the two models. Cadaver studies are more challenging to perform than the surrogate models, but are more realistic.

Materials and methods

Specimens

A fourth generation tibia was purchased from Sawbones Worldwide (SKU:3402 – overall length: 405 mm; tibia plateau diameter: 84 mm; distal tibia diameter: 58 mm; mid-shaft diameter: 10 mm – WA, USA) and a left cadaver leg including all the soft tissue from the knee below was obtained from Anatomy gifts registry (sex: male; age: 62; body weight: 56 kg – MD, USA). The host institute had all the required approvals to perform this study. A transverse osteotomy was performed in each model using an oscillating saw (DEWALT, MD, USA). In the surrogate model, the sawbone tibia was cut. In the cadaver leg, the tibia and fibula were divided using a minimally invasive technique that preserved the soft tissues. Both transections were made in the mid-diaphyseal region.

The tibiae in both cases were stabilized with an external fixator (Taylor Spatial Frame (TSF), Smith & Nephew plc, TN, USA). This is shown schematically in Figure 1. A two-ring TSF construct was used with two proximal half pins and two distal half pins with a 90° divergence between the pins on each ring. The external fixator was then extended to produce a 50 mm fracture gap in the surrogate model; this was to ensure that the bony fragments did not come into contact during the

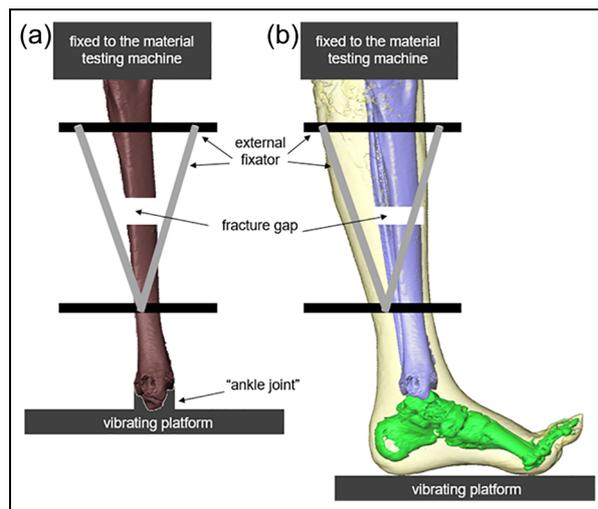


Figure 1. Schematic of the experimental set up in a lateral view: (a) the surrogate model and (b) the cadaver leg.

experimental loading. In the case of the cadaver specimen, a 13 mm fracture gap was produced, and further extension to match the surrogate model was not possible without overstretching the soft tissue (see Figure 1). This is a clinically typical fixation, although such fractures might be fixed with additional pins/wires pending various patient and injury-related factors. Considering that in this biomechanical study, the surrogate and cadaver models were fixed in the same configuration, the relative differences in outcome should remain valid.

Loading and measurements

The specimens were then fixed proximally to a material testing machine (Zwick Testing Machines Ltd., Herefordshire, UK) and distally rested on a commercial vibrating platform (Juvent, FL, USA – 0.3 g acceleration at 32–35 Hz with 0.05 mm vertical displacement). It must be noted that (1) the vibrating platform first finds the resonant frequency of the system and then initiates the vibrations, see the manufacturer website and previous studies describing and evaluating this system;^{20–22} (2) the natural frequency of a complete leg has been reported to be about 0.85 Hz²³ while we are not confident if this has been picked up by the vibrating platform but we are confident that the vibrating frequency applied by the platform is well away from the natural frequency of the leg. A titanium ‘foot’ was used to ensure direct contact between the surrogate tibia and the vibrating platform, while in the case of the cadaver leg, the specimen was in contact with the vibrating platform through the foot.

The specimens were loaded five times under static axial loads of 50, 100, 150 and 200 N equivalent to partial weight bearing.^{24,25} Note, normal limb loads are approximately of 3xBW, but the use of far lower loads here is due to the fact that the subjects do not weight bear significantly during distraction osteogenesis, and

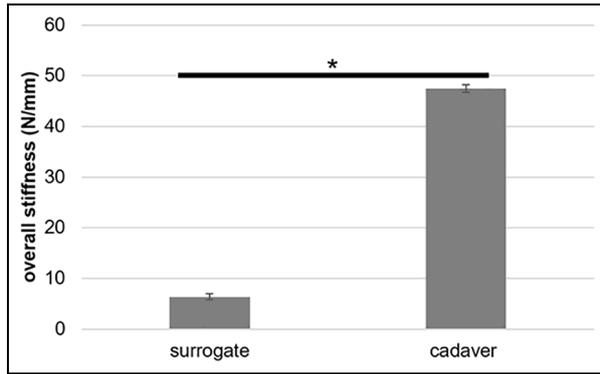


Figure 2. Overall stiffness of the fracture fixation constructs. Standard deviation is for five number of repeats of the axial compression test.

*Highlights significant difference.

are in line with measurements of frame loads carried out in author's lab.²⁶ At the end of each loading scenario, (1) the overall stiffness of the constructs were calculated based on the load-displacement data from the material testing machine; (2) the displacement at the fracture gap under the static loads was recorded with a calliper (with the resolution of 0.01 mm) on the lateral side and (3) the vibrating platform was turned on to vibrate the tibial shaft along its long axis. The fracture gap vibration (differential displacement across the medial fracture side) and the platform vibration were recorded using displacement sensors (with the resolution of 0.001 mm—DVRT, LORD MicroStrain, VT, USA) configured to LabVIEW (National Instruments, TX, USA).

Independent (two sample) t-test was used to compare the overall stiffness between the surrogate and cadaver models at 200 N loading. A dependent (paired) t-test was used to compare the difference between the displacement applied via the vibrating platform and the fracture movement both in the surrogate model and the cadaveric specimen. Significance level was set at $p < 0.05$.

Results

Static loading

The overall stiffness of the surrogate model was 6.39 ± 0.57 N/mm, and of the cadaver leg was 47.46 ± 0.74 N/mm, based on the load-displacement data at 200 N ($p < 0.05$). The fracture movement at the lateral side of the surrogate model and cadaver leg increased linearly ($R^2 = 0.9$) from 2.82 ± 0.13 mm and 0.23 ± 0.07 mm under 50 N to 10.99 ± 1.40 mm and 0.96 ± 0.08 mm under 200 N, respectively (Figure 3).

Dynamic loading

In the surrogate model, there was no significant difference between the displacement applied via the vibrating

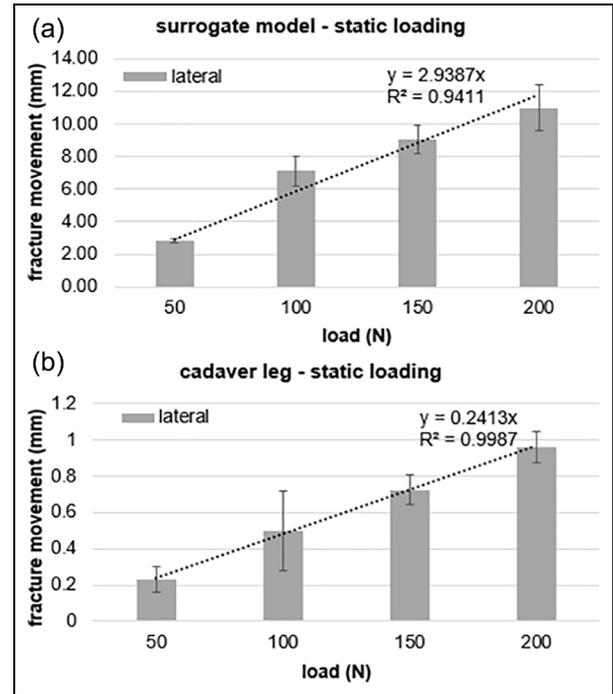


Figure 3. Fracture movement induced via static loading in (a) the surrogate model and (b) the cadaver leg.

platform (platform vibration) and the fracture movement induced at the fracture gap (fracture gap vibration) under each loading scenario, Figure 4. The displacement applied via the vibrating platform was however always higher than the fracture gap displacement. Average platform and fracture gap displacement (due to the vibration) across all loading scenarios were 0.030 ± 0.006 mm and 0.025 ± 0.008 mm, respectively (significant difference – $p < 0.05$; Figure 4).

In the cadaver leg, there was a statistically significant difference between the displacement applied via the vibrating platform (platform vibration) and the fracture movement induced at the fracture gap (fracture gap vibration) under each loading scenario. Average platform and fracture gap displacement (due to the vibration) across all loading scenarios were 0.027 ± 0.002 mm and 0.013 ± 0.003 mm, respectively (significant difference – $p < 0.05$; Figure 4).

There was found to be a significant difference between the amount of displacement of the vibrating platform between the surrogate model (0.030 ± 0.006 mm) and the cadaver leg specimen (0.027 ± 0.002 mm) during vibration across all loading scenarios.

Discussion

A tibial fracture, fixed with an external fixator, was tested experimentally in a surrogate model and a cadaveric leg. The constructs were statically loaded and then subjected to vibration with a commercial vibration platform, at each load interval, to quantify fracture

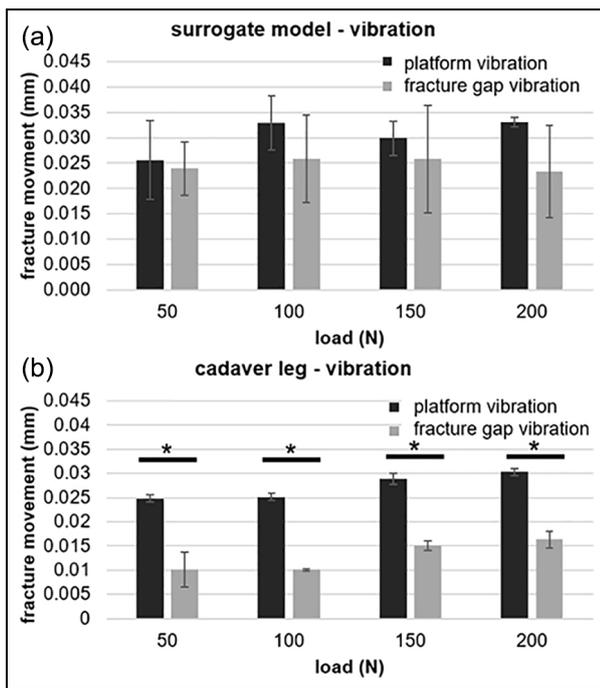


Figure 4. Fracture movement induced via the vibrating platform in (a) the surrogate model and (b) the cadaver leg. Standard deviation is for five number of repeats of the axial compression test.

*Highlights significant difference.

movement as a result of static loading and then with vibration.

The results highlighted a significant difference (eight times) between the overall stiffness of the surrogate model and the cadaveric leg (Figure 2). This is mainly due to the presence of soft tissues and the fibula in the cadaver model. However, other factors could have been contributing to the difference observed here. The frame constructs may not have been identically positioned resulting in different biomechanical properties.

A linear pattern of increase in fracture movement was observed in both cases due to the linear increase of loading from 50 to 200 N (Figure 3). However, there was about one order of magnitude difference between the fracture movement data obtained from the surrogate model and the cadaver leg. This was not surprising given the lower overall stiffness recorded for the surrogate model. In the case of the cadaver leg at 200 N, corresponding to partial weight bearing, fracture movement of 0.96 ± 0.08 mm was measured. This is within the acceptable 0.2–1 mm fracture movement that is suggested to promote callus formation and enhance the healing process.^{4,5,7,11} In distraction osteogenesis, the TSF is typically extended by 1 mm/day clinically. From Figure 3(b), this would correspond to 210 N at the bone ends. This seems to agree well with data from an instrumented fixator used in a clinical study,^{26,27} thus indicating that the stiffness of the cadaver tissues is likely to be similar to normal. Distal vibration of the tibia led to vibration at the fracture gap in both the surrogate model and cadaver

leg. In the cadaver leg, a significant difference was observed between the displacement applied via the vibrating platform (0.027 ± 0.003 mm – averaged over all tests) and the fracture movement (0.013 ± 0.003 mm – averaged over all tests; see Figure 4). The difference between the two displacements at the fracture gaps is likely to have been altered by the soft tissues in the cadaver leg and highlights the contribution made by the soft tissues to both static and dynamic stiffness.

This study has several limitations but perhaps the key limitation is that only one surrogate model and one cadaveric leg were used. While the study would have benefitted from a larger sample size, the authors think that the differences captured in this study will remain valid with a larger sample size. Note, considering that only one surrogate and one cadaver leg were used in this study (while several tests were carried out), statistical analysis data must be considered with caution. Further in vivo studies are required to test the hypothesis that WBV can improve the fracture healing process in humans and to investigate the effect of different frequencies, since only one frequency band was used here. Depending on the frequency and magnitude of the load, other vibrational regimes may also be osteogenic. In this article, we have chosen to investigate one level and suggest that this would be osteogenic.

In summary, this study has highlighted the effect of soft tissues in biomechanical studies. Soft tissues can alter the overall stiffness and fracture movement recorded in biomechanical studies investigating the effect of various devices or therapies. While the relative comparison between the devices or therapies may remain valid, absolute magnitude of recordings in such studies must be interpreted with caution.

Declaration of conflicting interests

The author(s) declared no potential conflicts of interest with respect to the research, authorship and/or publication of this article.

Funding

The author(s) disclosed receipt of the following financial support for the research, authorship and/or publication of this article: This work was supported by EPSRC-NIHR Healthcare Technology Co-operative (HTC) Partnership Award - UNIFY: A network focused on the treatment of fracture non-unions (EP/M000230/1) and UNIFY Plus (EP/N027221/1). Moazen was also supported by a Royal Academy of Engineering Research Fellowship (10216/119). We also thank Mr Arsalan Marghoub and Drs Chaorong Liu, Daniel Fong, Kaddour Bouazza-Marouf, Owen Davis and Alastair Campbell Ritchie.

ORCID iDs

Mehran Moazen  <https://orcid.org/0000-0002-9951-2975>

Jonathan Wright  <https://orcid.org/0000-0001-6055-648X>

References

- Zimmermann G and Moghaddam A. Trauma: non-union: new trends. In: Bentley G (ed.) *European instructional lectures*. Berlin: Springer, 2010, pp.15–19.
- Copuroglu C, Calori GM and Giannoudis PV. Fracture non-union: who is at risk? *Injury* 2013; 44: 1377–1672.
- Court-Brown CM and Caesar B. Epidemiology of adult fractures: a review. *Injury* 2006; 37: 691–697.
- Goodship AE and Kenwright J. The influence of induced micromovement upon the healing of experimental tibial fractures. *J Bone Joint Surg Br* 1985; 67: 650–655.
- Augat P, Merk J, Ignatius A, et al. Early, full weight bearing with flexible fixation delays fracture healing. *Clin Orthop Relat Res* 1996; 328: 194–202.
- Hak DJ. Management of aseptic tibial non-union. *J Am Acad Orthop Surg* 2011; 19: 563–573.
- Moazen M, Jones AC, Leonidou A, et al. Rigid versus flexible plate fixation for periprosthetic femoral fracture-computer modelling of a clinical case. *Med Eng Phys* 2012; 34: 1041–1048.
- Moazen M, Mak JH, Etchels LW, et al. The effect of fracture stability on the performance of locking plate fixation in periprosthetic femoral fractures. *J Arthroplasty* 2013; 28: 1589–1595.
- Leonidou A, Moazen M, Skrzypiec DM, et al. Evaluation of fracture topography and bone quality in periprosthetic femoral fractures: a preliminary radiographic study of consecutive clinical data. *Injury* 2013; 44: 1799–1804.
- Leonidou A, Moazen M, Lepetsos P, et al. The biomechanical effect of bone quality and fracture topography on locking plate fixation in periprosthetic femoral fractures. *Injury* 2015; 46: 213–217.
- Claes L, Wilke HJ, Augat P, et al. Effect of dynamization of gap healing of diaphyseal fractures under external fixation. *Clin Biomech* 1995; 8: 227–234.
- Egol KA, Kubiak EN, Fulkerson E, et al. Biomechanics of locked plates and screws. *J Orthop Trauma* 2004; 18: 488–493.
- Ogrodnik PJ, Moorcroft CI and Thomas PBM. A fracture movement monitoring system to aid in the assessment of fracture healing in humans. *Proc IMechE, Part H: J Engineering in Medicine* 2001; 215: 405–414.
- Leung KS, Shi HF, Cheung WH, et al. Low-magnitude high-frequency vibration accelerates callus formation, mineralization, and fracture healing in rats. *J Orthop Res* 2009; 27: 458–465.
- Kasturi G and Adler RA. Mechanical means to improve bone strength: ultrasound and vibration. *Curr Rheumatol Rep* 2011; 13: 251–256.
- Wehrle E, Liedert A, Heilmann A, et al. The impact of low-magnitude high-frequency vibration on fracture healing is profoundly influenced by the oestrogen status in mice. *Dis Model Mech* 2015; 8: 93–104.
- Harrison A, Lin S, Pounder N, et al. Mode & mechanism of low intensity pulsed ultrasound (LIPUS) in fracture repair. *Ultrasonics* 2016; 70: 45–52.
- Thompson WR, Yen SS and Rubin J. Vibration therapy: clinical applications in bone. *Curr Opin Endocrinol Diabetes Obes* 2014; 21: 447–453.
- Goodship AE, Lawes TJ and Rubin CT. Low-magnitude high-frequency mechanical signals accelerate and augment endochondral bone repair: preliminary evidence of efficacy. *J Orthop Res* 2009; 27: 922–930.
- Fritton JC, Rubin CT, Qin YX, et al. Whole-body vibration in the skeleton: development of a resonance-based testing device. *Ann Biomed Eng* 1997; 25(5): 831–839.
- Rubin C, Pope M, Fritton JC, et al. Transmissibility of 15-hertz to 35-hertz vibrations to the human hip and lumbar spine: determining the physiologic feasibility of delivering low-level anabolic mechanical stimuli to skeletal regions at greatest risk of fracture because of osteoporosis. *Spine* 2003; 28(23): 2621–2627.
- Alizadeh-Meghbrai M, Zariffa J, Masani K, et al. Variability of vibrations produced by commercial whole-body vibration platforms. *J Rehabil Med* 2014; 46(9): 937–940.
- Wagenaar RC and van Emmerik RE. Resonant frequencies of arms and legs identify different walking patterns. *J Biomech* 2000; 33: 853–861.
- Ryf CR and Arraf J. Postoperative fracture treatment: general considerations. In: Ruedi TP, Buckley RE and Moran CG (eds) *AO principle of fracture management*. 2nd ed. Davos: AO Publishing, 2007, p.447.
- Ganse B, Yang PF, Gardlo J, et al. Partial weight bearing of the tibia. *Injury* 2016; 47: 1777–1782.
- Laubscher M, El-Tawil S, Ibrahim I, et al. Measurement of forces across a Taylor Spatial Frame during activity. *Orthop Proc* 2015; 97-B(5): 15.
- Simpson AH, Cunningham JL and Kenwright J. The forces which develop in the tissues during leg lengthening. A clinical study. *J Bone Joint Surg Br* 1996; 78(6): 979–983.